

89/530684



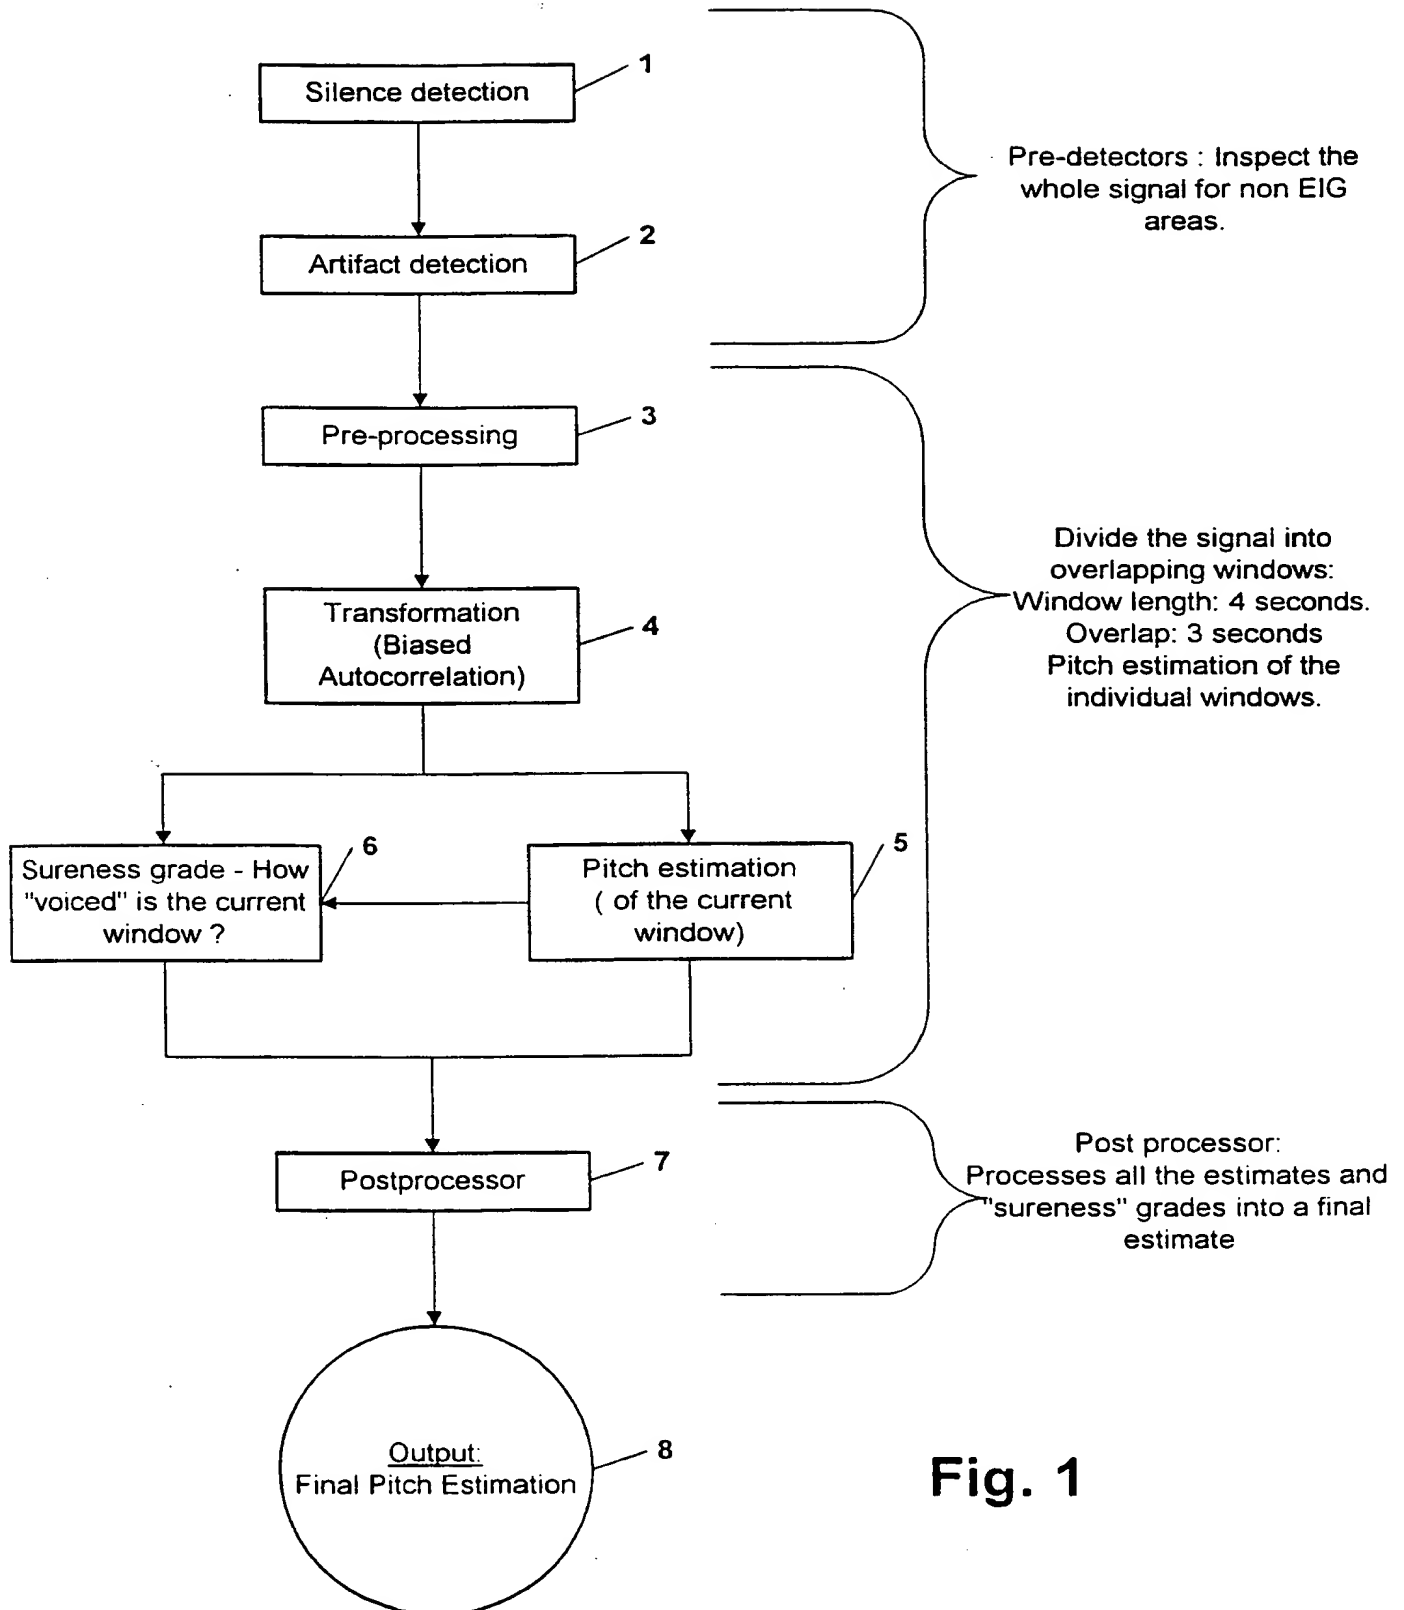


Fig. 1


09/530084

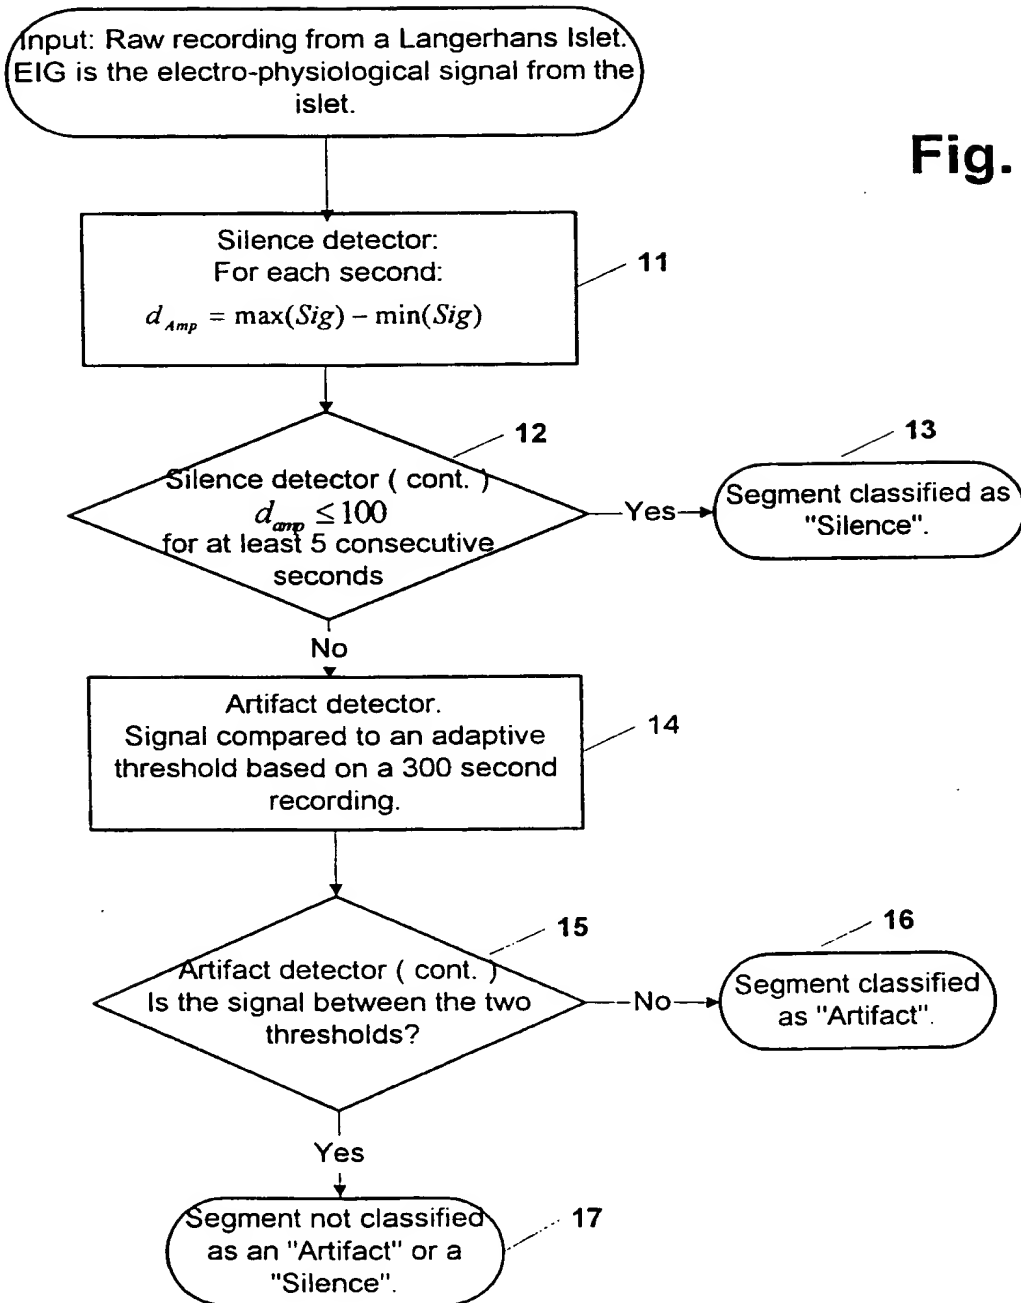

Note: The exact thresholds vary greatly due to the measurement methods, the measurement equipment, and the conditions of the experiment. The thresholds must be fitted manually for each experimental set-up.

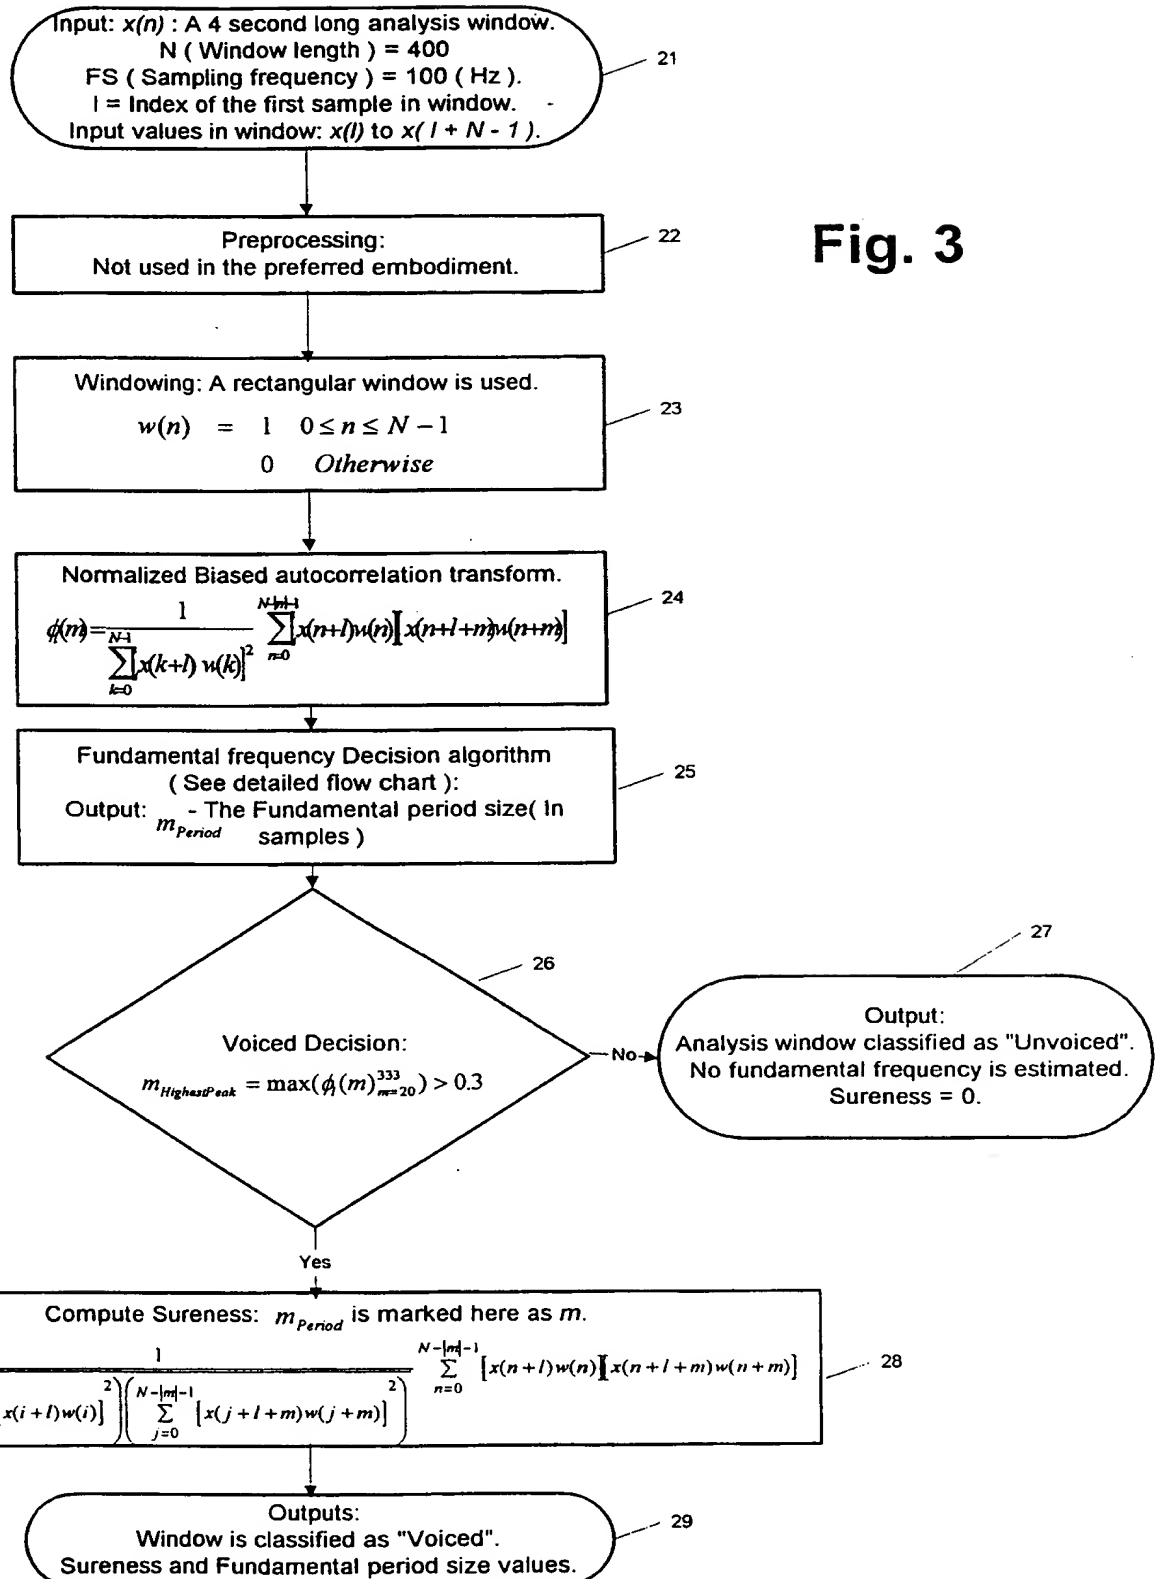

09/530684

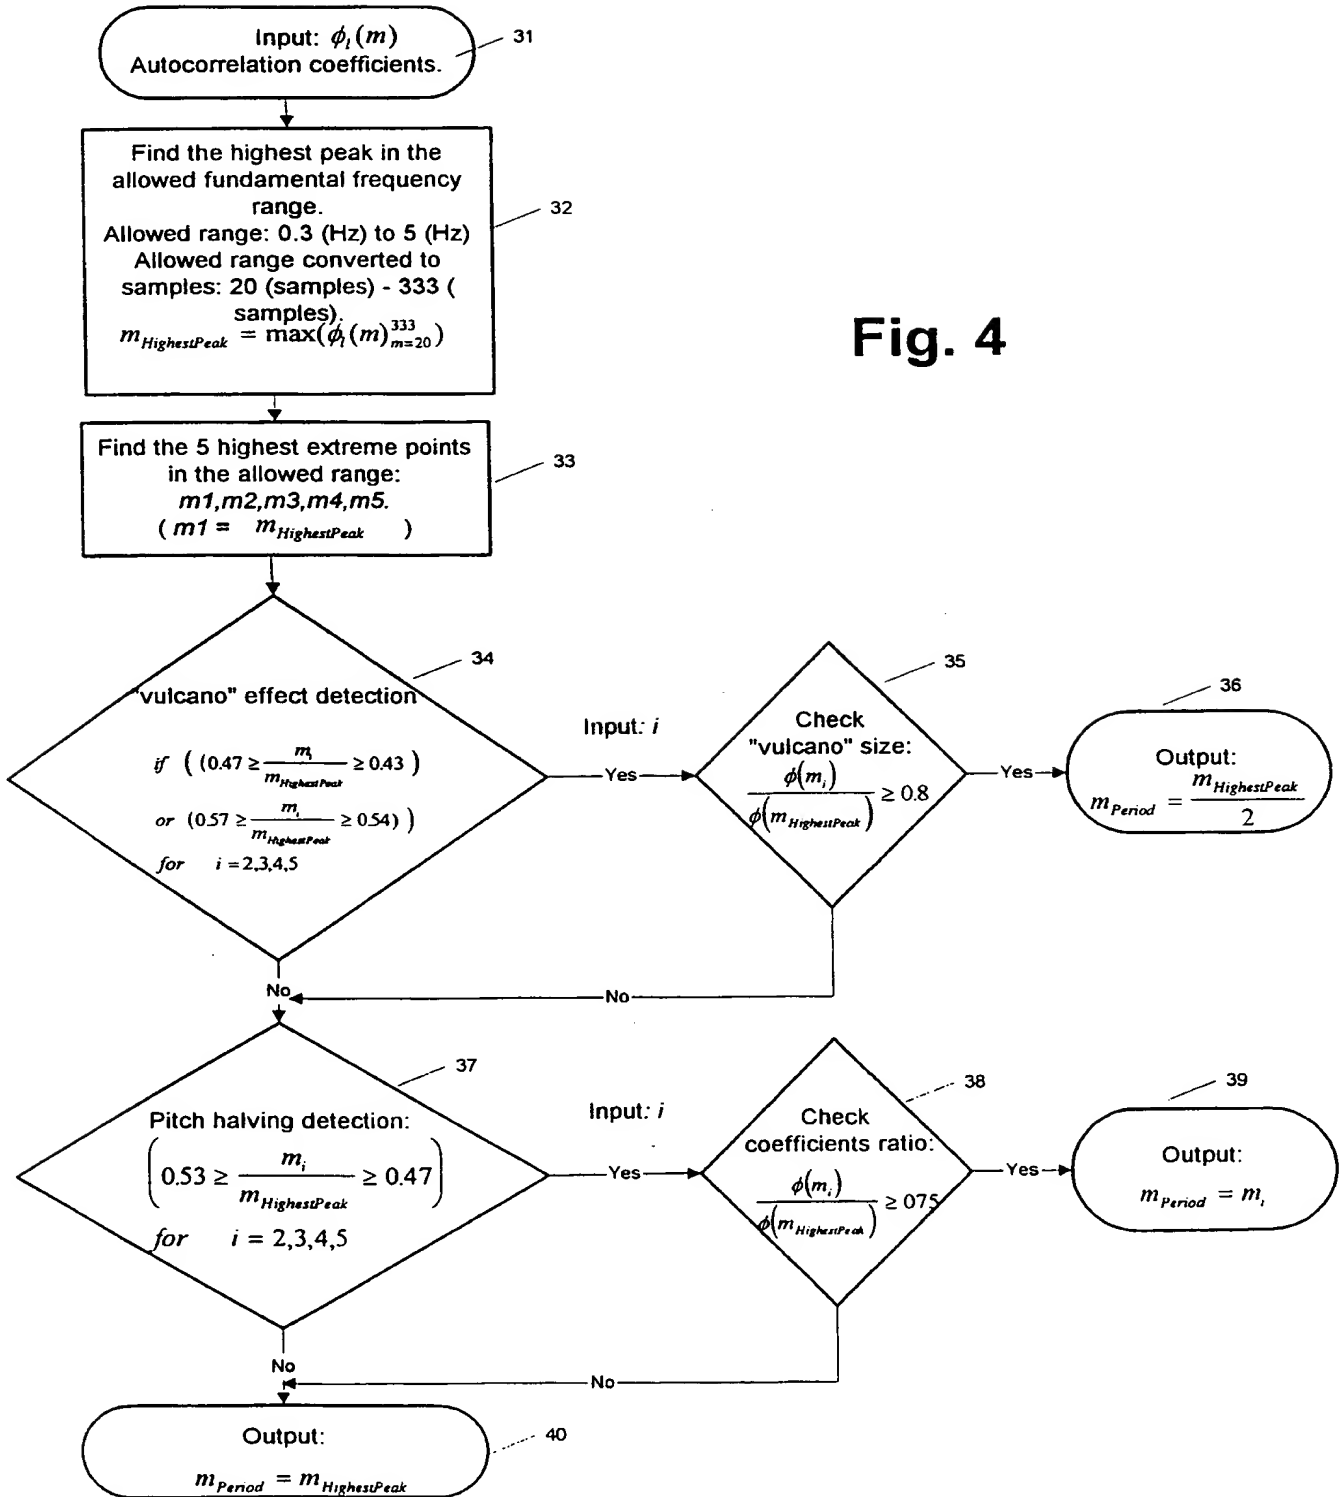

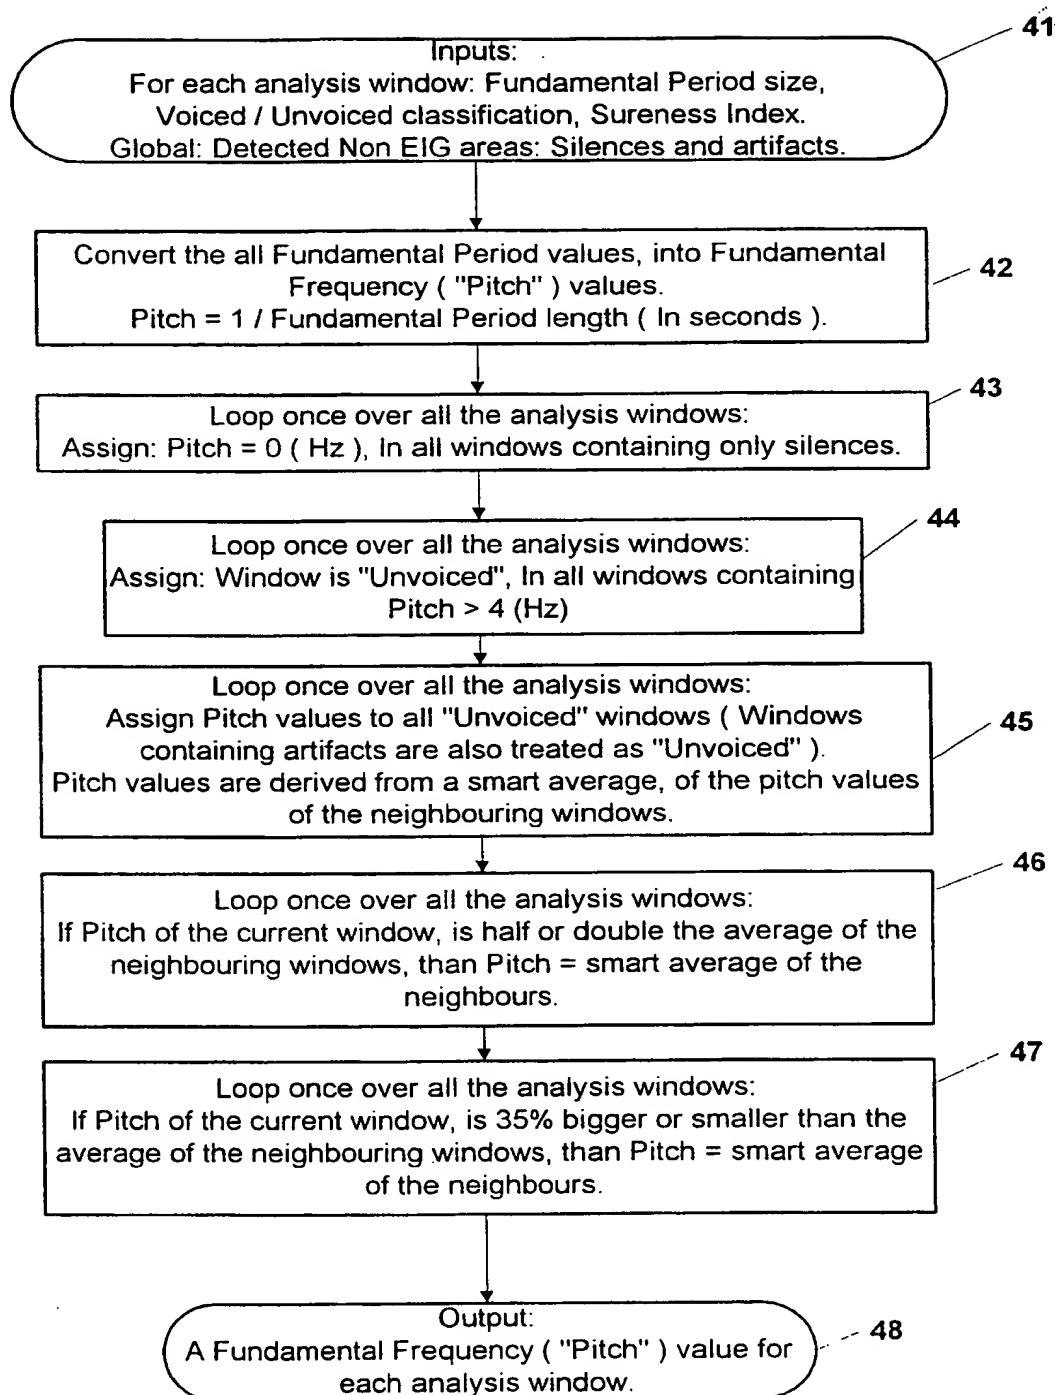


Fig. 5